

Sialic Acid Assay Kit (Colorimetric/Fluorometric)

LS-K293-100 (100 Tests) • See Storage Conditions Below



Introduction

SIALIC ACID is a general name for nine carbon acidic sugars with N- or O-substituted derivatives. The most common member of these sugars is N-acetylneuraminic acid (NANA). Sialic acid is widely distributed throughout mammalian tissues and fluids including serum. Sialylated oligosaccharides have been shown to exhibit antiviral properties and are also known to influence blood coagulation and cholesterol levels. The sialic acid level in body fluids is also an important marker for diagnosing cancer. Simple and direct procedures for measuring sialic acid concentrations find wide applications in research and drug discovery. This sialic acid assay uses an improved Warren Method, in which sialic acid is oxidized to formylpyruvic acid which reacts with thiobarbituric acid to form a pink colored product. The color intensity at 549 nm or fluorescence intensity at $\lambda_{ex/em} = 555/585$ nm is directly proportional to sialic acid concentration in the sample.

Key Features

- Sensitive and accurate. Use as little as 60 μ L samples. Linear detection range in 96-well plate: 5 to 1000 μ M sialic acid for colorimetric assays and 0.5 to 100 μ M for fluorometric assays.

Applications

- Direct Assays: sialic acid in biological samples (e.g. serum, plasma, saliva, milk).

Components

Component	K293-100
	100 Tests
Dye Reagent	6 mL
10% TCA	5 mL
DMSO	12 mL
Oxidation Reagent	10 mL
Hydrolysis Reagent	10 mL
Standard (10 mM Sialic Acid)	500 μ L

Materials Not Supplied

Pipetting devices, centrifuge tubes, centrifuge, heat block, clear flat-bottom 96-well plates, black 96-well plates (e.g. Corning Costar) and plate readers.

Storage

The kit is shipped at ambient temperature. Store the Standard at -20°C , all others at room temperature. Shelf life of twenty four months after receipt.

FOR RESEARCH USE ONLY! Not for use in humans.

LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121

www.LSBio.com • (206) 464-1554 • TechnicalSupport@LSBio.com

Sialic Acid Assay Kit (Colorimetric/Fluorometric)

LS-K293-100 (100 Tests) • See Storage Conditions Below



Assay Procedure

Colorimetric Procedure

- Standards. Equilibrate all components to room temperature. Prepare a 1000 μM sialic acid standard Premix by mixing 25 μL of the 10 mM Standard and 225 μL distilled water dH_2O . Dilute Standard as follows.

No	Premix + dH_2O	Vol (μL)	Sialic Acid (μM)
1	100 μL + 0 μL	100	1000
2	60 μL + 40 μL	100	600
3	30 μL + 70 μL	100	300
4	0 μL + 100 μL	100	0

Transfer 20 μL standards into four labeled Eppendorf tubes, add 5 μL 10% TCA.

- Samples treatment. To determine total sialic acid (TSA), samples need to be hydrolyzed to release bound sialic acid as follows. In an Eppendorf tube, mix 20 μL sample, 40 μL dH_2O and 40 μL Hydrolysis Reagent. Heat at 80°C for 60 min, let cool and briefly centrifuge. Add 25 μL 10% TCA, vortex and centrifuge at 14,000 rpm for 10 min. Transfer 25 μL supernatant into a clean tube and label it "TSA".

To determine free sialic acid (FSA), directly precipitate protein by mixing 40 μL sample and 10 μL 10% TCA. Vortex and centrifuge at 14,000 rpm for 10 min. Transfer 25 μL supernatant into a clean tube and label it "FSA".

- Oxidation. Prepare working reagent for each tube by mixing 15 μL Hydrolysis Reagent, 50 μL dH_2O and 65 μL Oxidation Reagent. Add 125 μL working reagent to each tube and let stand for 60 min at room temperature.
- Color Reaction. Add 50 μL Dye Reagent to each tube. Mix and heat for 10 min at 100°C. Let cool for another 5-10 min. Add 100 μL DMSO to each tube. Mix and centrifuge for 5 min at 14,000 rpm. Transfer 250 μL supernatant into separate wells of a clear, flat-bottom 96-well plate.
- Read optical density at 549 nm (540-555nm).

Fluorometric Procedure

The fluorometric assay is 10-fold more sensitive than the colorimetric assay. Prepare standards at 0, 30, 60 and 100 μM sialic acid in dH_2O .

The sample treatment, oxidation and color reaction steps are the same, except that the final reaction mixture is transferred into wells of a black, flat-bottom 96-well plate. Read fluorescence intensity at $\lambda_{\text{ex}} = 555$ nm and $\lambda_{\text{em}} = 585$ nm.

Calculations

Subtract blank value (#4) from the standard values and plot the ΔOD or ΔF against standard concentrations. Determine the slope and calculate the sialic acid concentration of Sample,

$$[\text{Sialic acid}] = \frac{R_{\text{SAMPLE}} - R_{\text{BLANK}}}{\text{Slope } (\mu\text{M}^{-1})} \times n \quad (\mu\text{M})$$

R_{SAMPLE} and R_{BLANK} are optical density or fluorescence intensity readings of the Sample and dH_2O Blank (#4), respectively. n is the sample dilution factor, $n = 5$ for TSA assays and $n = 1$ for FSA assays.

Note: if the Sample OD value is higher than that for the 1000 μM Standard, or sample fluorescence intensity higher than that for the 100 μM Standard, dilute sample in water and repeat the assay. Multiply result by the fold of dilution.

Conversions: 1000 μM NANA equals 30.9 mg/dL or 309 ppm.

FOR RESEARCH USE ONLY! Not for use in humans.


LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121

www.LSBio.com • (206) 464-1554 • TechnicalSupport@LSBio.com


Sialic Acid Assay Kit (Colorimetric/Fluorometric)

LS-K293-100 (100 Tests) • See Storage Conditions Below

Sample Data

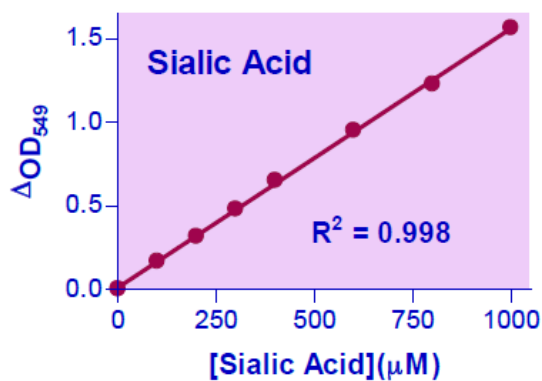

96-well colorimetric assay

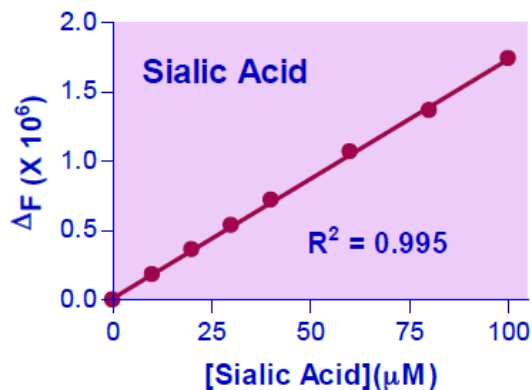

96-well fluorimetric assay

Version: V.08.09.2018

FOR RESEARCH USE ONLY! Not for use in humans.

LifeSpan BioSciences, Inc. • 2401 Fourth Avenue, Suite 900, Seattle, WA 98121

www.LSBio.com • (206) 464-1554 • TechnicalSupport@LSBio.com